



OMX 333DC




- Range $\pm 0.5/\pm 1/\pm 5$ A
 $\pm 25/\pm 50/\pm 100/\pm 200/\pm 400$ V
- Output 0/4...20 mA/0...5 mA/0...2/5/10 V/ ± 10 V
- Digital filters, Tare, Linearization
- Galvanic separation 2.5 kVAC
- Power supply 10...30 VDC / 24 VAC

Option

Comparators ● Data output

DIGITAL ISOLATED TRANSMITTER

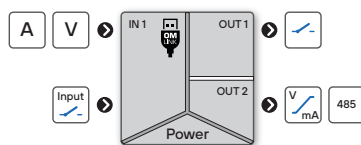

The OMX 333 model series are simple DIN rail mountable adjustable transmitters.

Type OMX 333DC is designed for measurements of higher DC and AC voltage and current, easily adjustable in the instrument's menu.

The instrument is based on a microcontroller and 16-bit ADC and DAC, which provides good accuracy, stability and ease of use.

OPERATION

Instrument can be controlled by two push buttons and a DIP switch located on the front panel. When frequent changes of settings are needed, we recommend the use of OM Link interface, which in conjunction with free control SW allows for modification and storage of all instrument's settings and also for firmware upload (using OM Link cable) from a PC.

The above mentioned SW can also be used for visualisation and archiving of measured values from a number of instruments via the RS 485 line.

All settings are stored in the EEPROM memory (they hold even after the instrument is switched off).

OPTION

COMPARATORS are assigned to monitor two limit values with relay output. The limits have adjustable hysteresis within the full range of the display as well as selectable delay of the switch-on in the range of 0...99.9 s. Reaching the preset limits is signalled by LED and simultaneously by the switch-on of the relevant relay.

DATA OUTPUTS are for their rate and accuracy suitable for transmission of the measured data for further projection or directly into the control systems. We offer an isolated RS485 with ASCII protocol.

STANDARD FUNCTIONS

PROGRAMMABLE INPUT

Measuring range: adjustable in menu

Teach-In: Min and Max values can be assigned to any two values of (unknown) input signal

ANALOG OUTPUT

Type: isolated, programmable with a resolution of 16 bit, rate < 0.2 ms

Ranges: 0...2/5/10 V/ ± 10 V, 0...5 mA/0/4...20 mA

FUNCTIONS

Linearization: non-linear signal is converted by a 25-point linear interpolation

Tare: designed to reset display upon non-zero input signal

DIGITAL FILTERS

Exponential average: from 2...100 measurements

Rounding: setting a „shorter“ number for further signal processing

EXTERNAL CONTROL

Hold: display/instrument blocking

Lock: control keys blocking

Tare: activation and tare resetting

TECHNICAL DATA

INPUT

No. of inputs	1	The range is adjustable in the instrument menu	
PM Range	±0.5 A	< 15 mV	Input 5
	±1 A	< 30 mV	Input 5
	±5 A	< 150 mV	Input 5
	±25 V	10 MΩ	Input 1
	±50 V	10 MΩ	Input 1
	±100 V	10 MΩ	Input 1
	±200 V	10 MΩ	Input 1
±400 V	10 MΩ	Input 1	

EXTERNAL INPUT

No. of inputs	1, on contact										
Function	<table border="0"> <tr> <td>OFF</td> <td>no function assigned</td> </tr> <tr> <td>HOLD</td> <td>measurement paused</td> </tr> <tr> <td>LOCK</td> <td>control keys blocking</td> </tr> <tr> <td>TARE</td> <td>tare activation</td> </tr> <tr> <td>CL. TA</td> <td>tare resetting</td> </tr> </table>	OFF	no function assigned	HOLD	measurement paused	LOCK	control keys blocking	TARE	tare activation	CL. TA	tare resetting
OFF	no function assigned										
HOLD	measurement paused										
LOCK	control keys blocking										
TARE	tare activation										
CL. TA	tare resetting										

INSTRUMENT SPECIFICATION

TC	50 ppm/°C
Accuracy	±0.1% of FS + 1 digit <i>above accuracies apply for 20 meas./s</i>
Rate	0.5..80 measurement/s
Overload	10x (t < 30 ms), 2x <i>not valid for > 200 V and 5 A ranges</i>
Functions	Teach-in, tare
Digital filters	exponential average, rounding
Linearization	linear interpolation in 25 points <i>setup only via OM Link</i>
OM Link	company communication interface for operation, setting and update of instruments (microUSB)
Watch-dog	reset after 500 ms
Calibration	at 25°C and 40 % rh.

RELAYS / OC OUTPUT

No. of outputs	up to 2
Type	digital, menu adjustable
Mode	HYSTER active above set value
Function Relays/OC	CLOSE is closed in active mode OPEN is open in active mode READY output indicates error-free status ERROR output indicates an error condition
Limits	..99999..999999
Hysteresis	0..999999
Delay	0..99.9 s
Outputs	1..2x relay with switch-on contact (Form A) (250 VAC/30 VDC, 3 A)* 1..2x open collector (30 VDC/100 mA)
Relays	1/8 HP 277 VAC, 1/10 HP 125 V, Pilot Duty D300

* values apply for resistance load

ANALOG OUTPUTS

No. of outputs	1
Type	isolated, adjustable with 16-bit DAC, output type and range is selectable
TC	15 ppm/°C
Non-linearity	0.1 % from FS
Accuracy	±0.02 % of FS
Rate	response to change of value < 1 ms
Ranges	0..2 / 5 / 10 V, ±10 V, resistive load ≥ 1 kΩ 0..5 / 20 mA / 4..20 mA, comp. < 600 Ω/12 V Indication of error message (output < 3.2 mA)

DATA OUTPUTS

No. of outputs	1
Protocol	ASCII
Data format	8 bit + no parity + 1 stop bit
Rate	300..230 400 Baud
RS 485	isolated, addressing (max. 31 instruments)

POWER SUPPLY

Range	10..30 V AC/DC, ±10 %, PF ≥ 0.4, I _{typ} < 40 A / 1 ms, isolated <i>Protection by fuse inside the device</i>
Consumption	< 2 W / 2 VA

MECHANIC PROPERTIES


Material	PA 66, incombustible UL 94 V-1, blue
Dimensions	25 x 79 x 90.5 mm (w x h x d)
Installation	on DIN rail, width 35 mm

OPERATING CONDITIONS

Connection	connector terminal blocks, section < 15 / 2.5 mm ²
Stabilization period	within 5 minutes after switch-on
Working temperat.	-20°..60°C
Storage temperat.	-20°..85°C
Working humidity	< 95 % r.v., non condensing
Protection	IP20
Construction	safety class I
EL safety	EN 61010-1, A2
Dielectric strength	2.5 kVAC per 1 min test between supply and input 2.5 kVAC per 1 min test between supply and analog output
Insulation resist.*	for pollution degree II, measuring cat. III power supply > 300 V (PI), 255 (DI) input, output > 300 V (PI)
EMC	EN 61326-1, Industrial area
Seismic qualification	IEC/IEEE 60980-344 Edition 1.0, 2020, par. 6, 9
Mechanical resistance	EN 60068-2-6 ed. 2:2008

* PI - Primary insulation, DI - Double insulation

CONNECTION

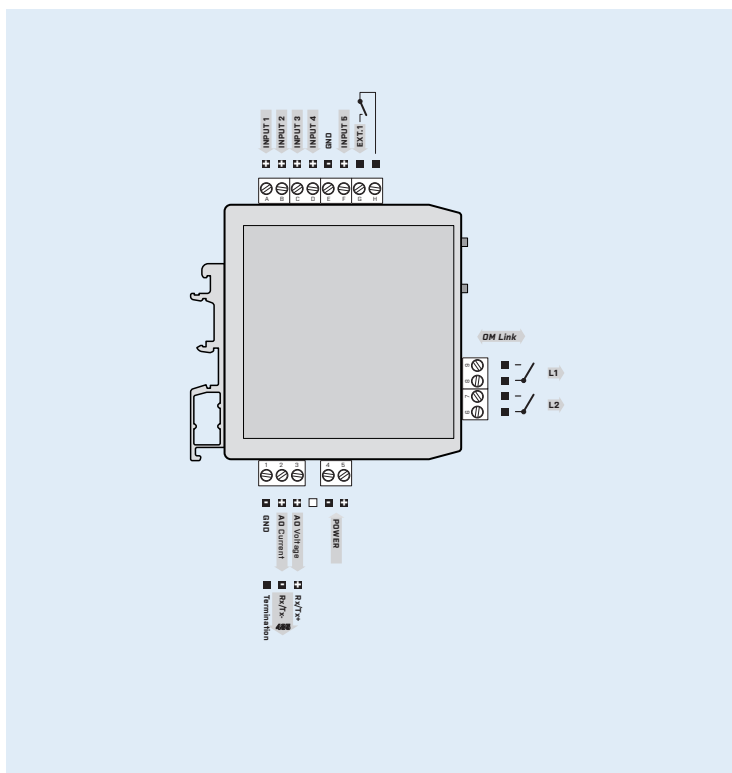

ORDER CODE

OMX 333DC

- [] - []

Comparators	no	0
	1x relay (Form A)	1
	2x relay (Form A)	2
	1x open collector	3
	2x open collector	4
Output	none	0
	analog	1
	RS 485	2
Specification	customized version, do not fill in	00

Basic configuration of the instrument is indicated in bold.