

OMX 333UQC



The OMX 333 model series are simple DIN rail mountable programmable transmitters.

Type OMX 333UQC is a universal transmitter - counter/frequency meter/timer/clock adjustable in the instrument's menu.

The instrument is based on a single-chip microcontroller, which provides good stability and ease of use.

PROGRAMMABLE ISOLATED TRANSMITTER

- Counter/Frequency/Clock/Timer
- Digital filters, Tare, Linearization, Sum
- Output: 0/4...20 mA/0...5 mA/0...2/5/10 V/±10 V
- Galvanic separation: 2,5 kVAC
- Power supply 10...30 VDC/24 VAC
- Option
Comparators - Data output

OMX 333UQC
UNIVERSAL COUNTER

OPERATION

Instrument can be controlled by two push buttons and a DIP switch located on the front panel. When frequent changes of settings are needed, we recommend the use of OM Link interface, which in conjunction with free control SW allows for modification and storage of all instrument's settings and also for firmware upload (using OM Link cable) from a PC.

The above mentioned SW can also be used for visualisation and archiving of measured values from a number of instruments via the RS 485 line.

All settings are stored in the EEPROM memory (they hold even after the instrument is switched off).

OPTION

COMPARATORS are assigned to monitor two limit values with relay output. The limits have adjustable hysteresis within the full range of the display as well as selectable delay of the switch-on in the range of 0...99,9 s. Reaching the preset limits is signalled by LED and simultaneously by the switch-on of the relevant relay.

DATA OUTPUTS are for their rate and accuracy suitable for transmission of the measured data for further projection or directly into the control systems. We offer an isolated RS485 with ASCII protocol.

STANDARD FUNCTIONS

PROGRAMMABLE INPUT

Setting: measuring mode counter/frequency with adjustable calibration coefficient and time base

Teach-In: Min and Max values can be assigned to any two values of (unknown) input signal

ANALOG OUTPUT

Type: isolated, programmable with a resolution of 16 bit, rate < 0,2 ms

Ranges: 0...2/5/10 V/±10 V, 0...5 mA/0/4...20 mA (comp. < 600 Ω)

FUNCTIONS

Linearization: non-linear signals can be linearized by the means of a linearization table (up to 25 points)

Tare: designed to reset display upon non-zero input signal

Preset: initial nonzero value that is always read after resetting the device

DIGITAL FILTERS

Exponential average: from 2...100 measurements

Rounding: setting the projection step for display

Input filter: passes the input signal up to 5...1 000 Hz

EXTERNAL CONTROL

Hold: display/instrument blocking

Lock: control keys blocking

Tare: activation and tare resetting

Resetting: counter resetting

TECHNICAL DATA

INPUT	
Number of inputs	1
UQC Input	optional in configuration menu on contact, TTL, NPN/PNP 0...30/300 V, comparison levels are adjustable in the menu (9.7 / 14.4 / 19.2 / 23.9 / 28.7 / 33.5 / 38.3 V) or automatic
Input frequency	0.1 Hz...50 kHz (Mode SINGLE) 0.1 Hz...20 kHz (Mode UP/DW) 0.1 Hz...20 kHz (Mode UP-DW) 0.1 Hz...20 kHz (Mode QUADR. - frequency) 0.1 Hz...10 kHz (Mode QUADR. - counter) (for duty cycle 50 %)
Measuring mode	SINGLE counter/frequency QUADR counter/frequency for IRC sensors UP/DW UP/DW counter/frequency and can display numbers/frequency UP - DW UP - DW counter/frequency and can display numbers/frequency TIME Timer RTC Clock
Time base	0.5/1/5/10 s
Multipl. constant	0,00001...999999
Dividing constant	0,00001...999999
Preset	0...999999
Input filter	0/5/40/100/1000 Hz allows you to set the maximum valid frequency that is being processed
Functions	Preset Summation Time backup (Timer/clock)
External input	1 input, on contact The following functions can be assigned: OFF input off HLD. display stop LOCK control keys blocking TAR. tare activation CLEAR display reset CLR.ST. reset/counter preset/timer CL.SUM. sum reset

INSTRUMENT ACCURACY
 TC: 50 ppm/°C
 Accuracy: ±0.01% of range
 Rate: 0.5...100 measurement/s
 Overload capacity: 2x; 10x (t < 30 ms)
 Digital filters: exponential average, rounding, 1/frequency, measurement to full speed (division constant)
 Functions: Tare
 Linearization: through linear interpolation in 25 points (only via OM Link)
 OM Link: company communication interface for operation, setting and update of instruments
 Watch-dog: reset after 500 ms
 Calibration: at 25°C and 40 % r.h.

COMPARATOR
 Type: digital, menu adjustable, contact switch-on < 50 ms
 Hysteresis mode: switching limit, hysteresis band (Lim and ±1/2 Hys.) and time (±99,9 s) determining the switching delay
 Mode C-Puls - automatic counter resetting at the set value
 Mode Once - switching limit, which will switch off only after the counter has been reset
 Mode On Run - output is active when the timer is running
 Output: 1...2x Form A relays (250 VAC/30 VDC, 3 A);
 1...2x open collector (30 VDC/100 mA)

DATA OUTPUTS
 Protocol: ASCII
 Data format: 8 bit + no parity + 1 stop bit (ASCII)
 Rate: 600...230 400 Baud
 RS 485: isolated, addressing (max. 31 instruments)

ANALOG OUTPUTS
 Type: isolated, programmable with a 16 bit D/A converter, type and range are selectable in menu
 Non-linearity: 0.1% of range
 TC: 15 ppm/°C
 Rate: response to change of value < 1 ms
 Ranges: 0...2/5/10 V, ±10 V, 0...5 mA, 0/4...20 mA
 (comp. < 600 Ω/12 V)
 Ripple: 5 mV residual ripple at output voltage of 10 V


POWER SUPPLY
 Range: 10...30 VDC/24 VAC, ±10 %, PF≥0.4, I_{STP}< 40 A/1 ms
 10...30 VDC/24 VAC, ±10 %, PF≥0.4, I_{STP}< 40 A/1 ms, isolated
 Consumption: < 2 W/2 VA

MECHANIC PROPERTIES
 Material: PA 66, incombustible UL 94 V0, blue
 Dimensions: 25 x 79 x 90.5 (w x h x d)
 Installation: on DIN rail, width 35 mm

OPERATING CONDITIONS
 Connection: connector terminal blocks, section < 1.5 mm²
 Stabilization period: within 5 minutes after switch-on
 Working temperature: -20°...60°C
 Storage temperature: -20°...80°C
 Protection: IP20
 E1. safety: EN 61010-1, A2
 Dielectric strength: 2.5kV per 1 min test between power supply, inputs and outputs
 Insulation resistance: for pollution degree II, measuring cat. III
 power supply > 550 V (PI), 255 V (DI)
 EMC: EN 61326-1

PI - Primary insulation, DI - Double insulation

CONNECTION

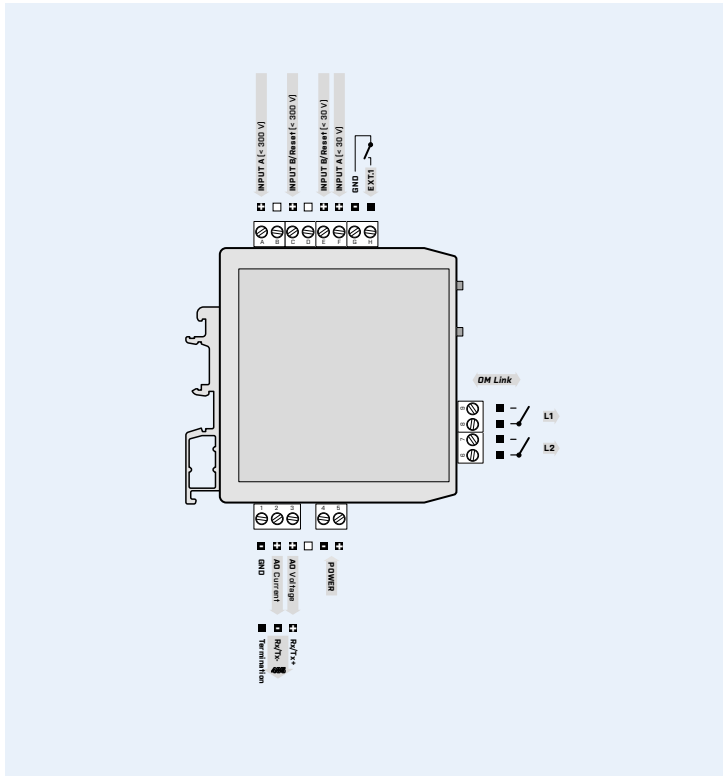

ORDER CODE

OMX 333UQC - - - -

Power supply	10...30 VDC/24 VAC	0		
	10...30 VDC/24 VAC, isolated	1		
Comparators	no		0	
	1x relay (Form A)		1	
	2x relay (Form A)		2	
	1x open collector		3	
	2x open collector		4	
Output	none		0	
	analog		1	
	RS 485		2	
Specification	customized version, do not fill in			00

Basic configuration of the instrument is indicated in bold.