



OM 351

3 1/2 DIGIT PROGRAMMABLE

DC VOLTMETER/AMMETER

AC VOLTMETER/AMMETER

PROCESS MONITOR


OHMMETER

THERMOMETER FOR PT 100/500/1 000

THERMOMETER FOR NI 1 000

THERMOMETER FOR THERMOCOUPLES

DISPLAY INST. FOR LINEAR POTENTIOMETERS

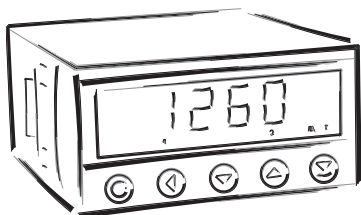

SAFETY INSTRUCTIONS

Please, read the enclosed safety instructions carefully and observe them!
These instruments should be safeguarded by isolated or common fuses (breakers)!
For safety information the EN 61 010-1 + A2 standard must be observed.
This instrument is not explosion-safe!

TECHNICAL DATA

Measuring instruments of the OM 351 series conform to the European regulation 89/336/EWG and the Ordinance 168/1997 Coll.

They are up to the following European and Czech standards:

CNS EN 55 022, class B

CNS EN 61000-4-2, -4, -5, -6, -8, -9, -10, -11

The instruments are applicable for unlimited use in agricultural and industrial areas.

CONNECTION

Supply of energy from the main line has to be isolated from the measuring leads.



ORBIT MERRET, spol. s r.o.

Vodňanská 675/30

198 00 Prague 9

Czech Republic

Tel: +420 - 281 040 200

Fax: +420 - 281 040 299

e-mail: orbit@merret.cz

www.orbit.merret.cz



1.	Contents	3
2.	Instrument description	4
3.	Connection	6
4.	Setting	8
	Symbols used in the instructions	10
	Setting the DP and the (-) sign	10
	Control keys functions	11
	Configuration of user menu items	11
5.	Setting "LIGHT" menu	12
5.0	Description "LIGHT" menu	12
	Setting input type "DC"	14
	Setting input type "AC"	16
	Setting input type "PM"	18
	Setting input type "DU"	20
	Setting input type "OHM"	22
	Setting input type "RTD"	24
	Setting input type "T/C"	26
	Setting the limits	28
	Setting the analog output	29
	Setting the menu type (LIGHT/PROFI)	30
	Restoration of the manufacture setting	30
	Calibration of the input range (DU)	31
	Setting new access password	32
	Instrument identification	32
6.	Setting "PROFI" menu	38
6.0	Description "PROFI" menu	38
6.1	"PROFI" menu - INPUT	
6.1.1	Tare resetting	38
6.1.2	Setting the measuring range, displacement, compensation and measuring rate	39
6.1.3	Setting the external control input	42
6.1.4	Setting functions of the control key [ENTER]	43
6.2	"PROFI" menu - CHANNELS	
6.2.1	Projection on the display (MIN, MAX)	44
6.2.2	Setting the digital filters	45
6.2.3	Setting the decimal point	45
6.3	"PROFI" menu - OUTPUT	
6.3.1	Configuration and setting the limits	46
6.3.2	Setting the data output	47
6.3.3	Setting the analog output	48
6.3.4	Setting the display brightness	49
6.4	"PROFI" menu - SERVICE	
6.4.1	Selection of the type of programming menu	50
6.4.2	Restoration of the manufacture setting	51
6.4.3	Calibration of the input range (DU)	51
6.4.4	Setting new access password	51
6.4.5	Instrument identification	52
7.	Setting "USER" menu	54
7.0	Configuration "USER" menu	54
8.	Method of measuring of the cold junction	56
9.	Data protocol	57
10.	Error statements	58
11.	Technical data	60
12.	Instrument dimensions and installation	62
13.	Certificate of guarantee	63

2.1 DESCRIPTION

The OM 351 model series are 3 1/2 digit programmable panel instruments, manufactured in the following alternatives:

OM 351DC	DC voltmeter/ammeter
OM 351AC	AC voltmeter/ammeter
OM 351PM	Process monitor
OM 351RTD	Thermometer for Pt 100/500/1 000, Ni 1 000
OM 351T/C	Thermometer for thermocouples
OM 351DU	Display instrument for linear potentiometers
OM 351OHM	Ohmmeter

The instruments are based on an 8-bit microcontroller with A/D converter, which secures high accuracy, stability and easy operation of the instrument.

Programmable projection of the display

Setting	selection of measuring range
Calibration	projection for both limit values of the input signal
Projection	±1999

Linearisation

Linearisation through linear interpolation in 25 points (pouze přes OM Link)**

Compensation of

Conduct	automatic compensation of 2-wire conduct
Probes measuring head)	compensation of internal resistance of the measuring probe (conduct resistance in the
Cold junctions	fixed or automatic

Digital filters

Rounding	setting the projection step for display
Exponen. average	from 2...100 measurements

Mathematic functions

Tare*	assigned to reset display in case of non-zero input signal
-------	--

External control

Hold	display/instrument blocking
Lock	locking the control keys for access into Configuration menu
Tára*	tare activation

* only for types DC, PM **only for types DC, PM, OHM, DU

2.2 OPERATION

The instrument is set and controlled by five control keys located on the front panel. All programmable settings of the instrument are realized in two adjusting modes:

- LIGHT** Simple programming menu
- contains only items necessary for instrument setting and is protected by an optional numeral code
- PROFI** Complete programming menu
- contains complete instrument menu and is protected by an optional numeral code
- USER** User programmable menu
- may contain arbitrary items selected from programmable menu (LIGHT/PROFI), which determines the authorization (see or change)
 - access is without password

All programmable parameters are stored in the EEPROM memory (they hold even after the instrument is switched off).



Complete operation and setting of the instrument may be performed via communication interface OM Link, which is a standard equipment of every instrument.

The operation program is freely available (www.orbit.merret.cz) and the only requirement is the purchase of OML cable for connecting the instrument to PC. It is manufactured in version RS 232 and USB and is compatible with all ORBIT MERRET instruments.

Another option for connection is with the aid of data output RS 232 or RS 485 (without the need for OML cable).

The OM LINK program version „Standard“ allows you to connect an unlimited number of instruments with the option of visualization and storage in PC.

2.3 EXTENSION

Excitation is suitable for feeding sensors and converters. It has a galvanic isolation.

Comparators are assigned to control two limit values with relay output. The limits have adjustable hysteresis as well as selectable delay of the switch-on. Reaching the preset limits is signalled by LED and simultaneously by the switch-on of the relevant relay.

Data outputs are for their rate and accuracy suitable for transmission of measured data for further projection or directly into the control systems. We offer an isolated RS232 and RS485 with the ASCII protocol.


Analog outputs will find their place in applications where further evaluating or processing of measured data in external devices is required. We offer a universal analog output with the option of selection of output type - voltage/current. The value of analog output corresponds with the displayed data and its type and range are selectable in the programming mode.

3 INSTRUMENT CONNECTION


The lead for feeding of the instrument should not be in the proximity of incoming low-potential signals. Contactors, motors with larger input power and other efficient elements should not be in the proximity of the instrument.

The lead into instrument input (the measured quantity) should be in sufficient distance from all power leads and appliances. Provided this cannot be secured, it is necessary to use shielded leads with connection to ground (terminal E).

The instruments are tested in compliance with standards for use in industrial area, yet we recommend to abide by the above mentioned principles.

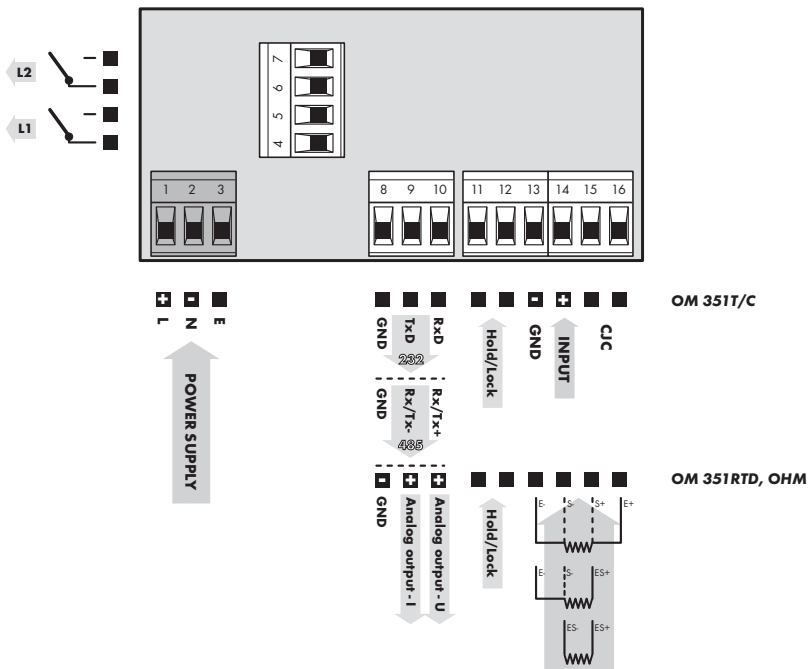

!
 Grounding on terminal „E“ has to be connected at all times.
 In case of RTD and OHM inputs with 2- or 3-wire connection it is necessary to link the unconnected inputs on the terminal board (13+14/15+16 or 15+16).

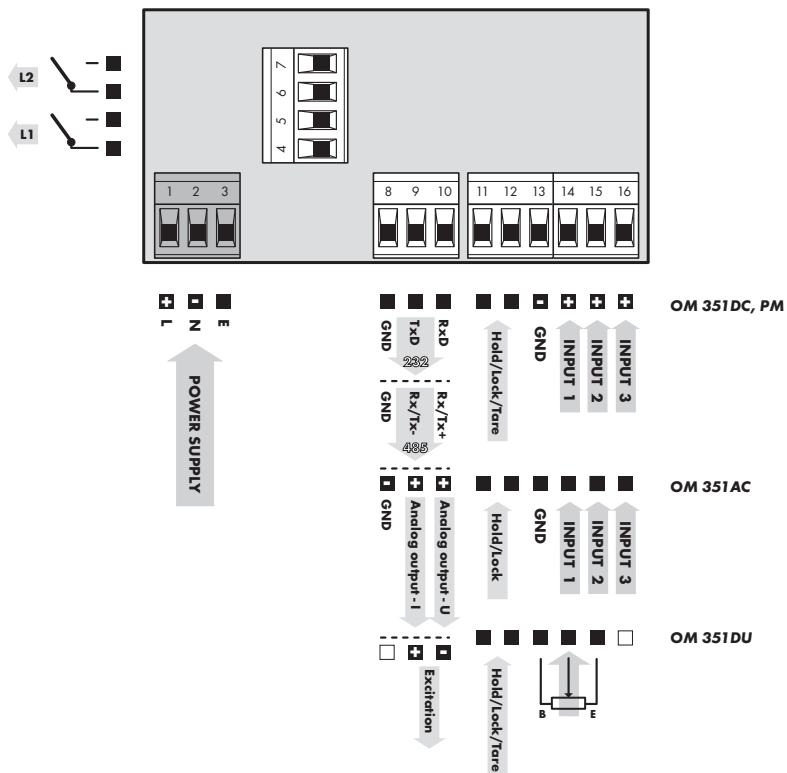

MEASURING RANGES

Type/Input	Input 1	Input 2	Input 3
OM 351 AC	0...60/150/300 mV	0...10 V	0...120 V
OM 351 AC	0...1 (2,5)/5 A	0...250 V	0...450 V
OM 351 DC	$\pm 2/\pm 20$ mA	$\pm 0,2/\pm 2$ V	$\pm 20/\pm 200$ V
OM 351 DC	0...1/5 A	0...60/150 mV	
OM 351 PM	0/4...20 mA	0...2 V	0...5/10 V
OM 351 OHM	0...200 Ohm * 0...2 kOhm * 0...100 kOhm * 5...105 Ohm		

SETTING
PROFI*profi*

- ▶ For expert users
- ▶ Complete instrument menu
- ▶ Access is password protected
- ▶ Possibility to arrange items of the „User“ menu

SETTING
LIGHT*light*

- ▶ For trained users
- ▶ Only items necessary for instrument setting
- ▶ Password protected access
- ▶ Possibility to arrange items of the „User“ menu

SETTING
USER*profi light**user*

- ▶ For user operation
- ▶ Menu items are set by the user (Profi/Light) as per request
- ▶ Access is not password protected
- ▶ Optional menu structure either tree (PROFI) or linear (LIGHT)

4.1 DESCRIPTION

The instrument is set and controlled by means of five control keys located on the front panel. All programmable settings of the instrument are realised in three adjusting modes:


- LIGHT** Simple programming menu
- contains only items necessary for instrument setting and is protected by an optional numeral code
- PROFI** Complete programming menu
- contains complete instrument menu and is protected by an optional numeral code
- USER** User programmable menu
- may contain arbitrary items selected from programmable menu (LIGHT/PROFI), which determines the authorization (see or change)
 - access is without password

Complete operation and setting of the instrument may be performed via communication interface OM Link, which is a standard equipment of every instrument.

The operation program is freely available (www.orbit.merret.cz) and the only requirement is the purchase of OML cable for connecting the instrument to PC. It is manufactured in version RS 232 and USB and is compatible with all ORBIT MERRET instruments.

Another option for connection is with the aid of data output RS 232 or RS 485 (without the need for OML cable).

Setting and controlling the instrument is performed by means of 5 control keys located on the front panel. With the aid of these keys it is possible to browse through the operation menu and to select and set required values.

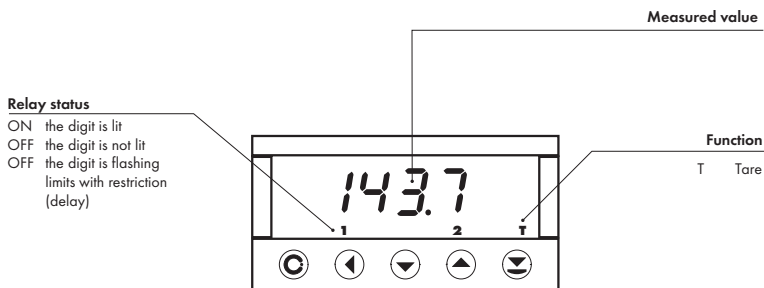

SYMBOLS USED IN THE INSTRUCTIONS

DC **AC** **PM**
DU **OHM** **RTD** **T/C** Indicates the setting for given type of instrument

DEF values preset from manufacture

symbol indicates a flashing light (symbol)

inverted triangle indicates the item that can be located into USER menu

after pressing the key the set value will not be stored

after pressing the key the set value will be stored

30 continues on page...

SETTING THE DECIMAL POINT AND THE MINUS SIGN

DECIMAL POINT

Its selection in the menu, upon modification of the number to be adjusted it is performed by the control key with transition to beyond the highest decade, when the decimal point starts flashing. Positioning is performed by / .

THE MINUS SIGN

Setting the minus sign is performed by the key on higher decade. When editing the item subtraction must be made from the current number (e.g.: 013 > , on class 100 > -87)

CONTROL KEYS FUNCTIONS

Key	Measurement	Menu	Setting numbers/Selection
	access into USER menu	exit menu w/o saving	transition to next item w/o saving
	tare value (DC, PM) resistance measured (RTD) cold junctions temperature (T/C)	back to previous level	move to higher decade
	cancel Tare	move to previous item	move down
	cancel Tare	move to next item	move up
	Tare	confirm selection	setting/selection confirmation
+	access into LIGHT/PROFI menu		
+	direct access into PROFi menu - temporary (remains LIGHT)		
+			configuration of an item for USER menu

CONFIGURATION OF USER MENU ITEMS

- in LIGHT or PROFi menu
- no items permitted in USER menu from manufacture
- on items marked by inverted triangle

nápis bliká - zobrazí se aktuální nastavení



n0

item will not be displayed in USER menu

YES

item will be displayed USER menu with the option of setting options

SH0

item will be solely displayed in the USER menu

5.0

SETTING "LIGHT"

LIGHT

Simple programming menu

- contains only items necessary for instrument setting and is protected by optional numeral code

SETTING LIGHT



- For capable users
- Only items necessary for instrument setting
- Password protected access
- Possibility to arrange items of the „User“ menu
- Linear menu structure

Preset from manufacture

Password	"0"
Menu	LIGHT
USR menu	off
Setting the items	DEF

1428



PAR5

0

Access code



Upon delay exceeding 30 s the programming mode is automatically discontinued and the instrument itself restores the measuring mode

Selecting input, range, projection

DC	NOd	14	nl_n	000	NAH	100.0
AC						
PM	FOR	00.0				
DU	nl_n	000	NAH	100.0	FOR	00.0
OHM	CO_n	0	nl_n	000	NAH	100.0
	FOR	00.0				
RTD	CO_n	0	FOR	00.0		
T/C	NOd	E	CO_n	ln. 1	t.C.D.	0

L1

250

L2

100.0

Extension - comparator

tYPE

120

RLo

0

Extension - Analog output

R.H.1

0

Menu type

nU

L10

Return to manufacture setting

rES

YES

DU

CLo

YES

CH.1

YES

Calibration - only for OM 351DU

New password

n.PR

0

Identification

Id

YES

00351...

1428

Return to previous measuring mode

1428



PAS



0

Setting for minimum
input signal

PAS Access into instrument menu

DC AC PM DU OHM RTD T/C

PAS = 0
- access into the Menu is unrestricted, after releasing keys you automatically move to first item of the menu

Set "Password" = 42 Example

0 1 2 0.2 2 2.2

2 4.2 n0d

OM 351AC	16
OM 351DC	18
OM 351PM	18
OM 351DU	18
OM 351OHM	20
OM 351RTD	22
OM 351T/C	24

OM 351DC



n0d

0.2 U 2 U 20 U 199 U 2 I 20 I

60 150 1 A 5 A

DC

n0d Selecting the instrument measuring range

- setting the input range depends on ordered measuring range

- **DEF** = 20. U
- **DEF** = 1. A

Menu	Range „A“	Range „B“
0.2U	±0.2 V	
2.U	±2 V	
20.U	±20 V	
199.U	±199 V	
2. i	±2 mA	
20. i	±20 mA	
60.		±60 mV
150.		±150 mV
1. A		±1 A
5. A		±5 A

Range ±20 V Example

0.2U 2U 20U nIn



Min Setting display projection for minimum value of input signal

- positioning the decimal point does not have effect on display projection
- after confirmation of the value the decimal point automatically moves to max. number of decimal places
- range of the setting is ± 1999
- **DEF** = 0

Projection for 0 V > Min = 0,23 Example

+ 000	+ 00	+ .002	+ .003	+ 003	+ 013
+ 023	+ .023	+ .023	+ .023	+ .023	ERR



Max Setting display projection for maximum value of input signal

- positioning the decimal point does not have effect on display projection
- after confirmation of the value the decimal point automatically moves to max. number of decimal places
- range of the setting is ± 1999
- **DEF** = 100

Projection for 20 V > Max = 800 Example

+ 100.0	+ 100.0	+ 100.0	+ 90.0	+ 80.0	+ 080.0
+ 080.0	+ 080.0	+ 080.0			ERR



FDR Setting projection of decimal point

- positioning of decimal point in measuring mode on the display is set here
- **DEF** = 0

Projection of decimal point on the display > XXX.x Example

000	000	ERR
-----	-----	-----

following item of the menu depends on instrument equipment

OM 351AC



nDd Selecting the instrument measuring range

- setting the input range depends on ordered measuring range
- **DEF** = U 1.

Menu	OM 351AC	
	Range „S“	Range „U“
U 1.	0...10 V	0...250 V
U 2.	0...120 V	0...450 V
Menu	Range „K“	Range „P“
I 1.	0...60 mV	0...1 A
I 2.	0...150 mV	0...2,5 A
I 3.	0...300 mV	0...5 A

Range 0...5 A

Example

U 1 U 2 I 1 I 2 I 3 nIn



nIn Setting display projection for minimum value of input signal

- range of the setting is ± 1999
- **DEF** = 0

- positioning the decimal point does not have effect on display projection
- after confirmation of the value the decimal point automatically moves to max. number of decimal places

Projection for 0 A > Min = 0

Example

+ 000 nRH



ARR Setting display projection for maximum value of input signal

- range of the setting is ± 1999
- **DEF** = 100

- positioning the decimal point does not have effect on display projection
- after confirmation of the value the decimal point automatically moves to max. number of decimal places

Projection for SA > Max = 350

Example

+ 100.0	+ 100.0	+ 10.0	+ 100.0	+ 103.0	+ 103.0
+ 105.0	+ 105.0	+ 115.0	+ 125.0	+ 135.0	+ 135.0
+ 035.0	+ 035.0	+ 035.0	+ 035.0	FOp	



FOP Setting projection of decimal point

- **DEF** = 0

- positioning of decimal point in measuring mode on the display is set here

Projection of decimal point on the display > XXXX.

Example

000	000	000	000	000	000	* following item of the menu depends on instrument equipment
-----	-----	-----	-----	-----	-----	--

OM 351PM



n0d

Selecting the instrument measuring range

- setting the input range depends on ordered measuring range
- **DEF** = 1 4

Menu	Range
U 2.	0...2 V
U 5.	0...5 V
U 10.	0...10 V
I 0.	0...20 mA
I 4.	4...20 mA

Range 4...20 mA

Example

U 2 I 4 n In

n In

Setting for minimum input signal

n In

Setting display projection for minimum value of input signal

- range of the setting is ± 1999
- **DEF** = 0

- positioning the decimal point does not have effect on display projection
- after confirmation of the value the decimal point automatically moves to max. number of decimal places

Projection for 4 mA > Min = -25

Example

+ 001 + 001 + 002 + 003 + 004 + 005

+ 005 - 005 - 005 - 025 - 025 - 025

n In



PMH Setting display projection for maximum value of input signal

- positioning the decimal point does not have effect on display projection
- after confirmation of the value the decimal point automatically moves to max. number of decimal places

- range of the setting is ± 1999

- **DEF** = 100

Projection for 20 mA > Max = 250 Example

+ 100.0	+ 100.0	+ 101.0	+ 102.0	+ 103.0	+ 104.0	+ 105.0
+ 105.0	+ 115.0	+ 125.0	+ 125.0	+ 025.0	+ 025.0	+ 025.0
+ 025.0	+ 025.0	FDr				



FDr Setting projection of decimal point

- positioning of decimal point in measuring mode on the display is set here

- **DEF** = 0

Projection of decimal point on the display > XXX.x Example

000.	000.	FDr	
------	------	-----	--

* following item of the menu depends on instrument equipment

OM 351DU



nIn Setting display projection for minimum value of input signal

- range of the setting is ± 1999
- **DEF** = 0

Projection for počátek > Min = 0

Example



- positioning the decimal point does not have effect on display projection
- after confirmation of the value the decimal point automatically moves to max. number of decimal places



nRH Setting display projection for maximum value of input signal

- range of the setting is ± 1999
- **DEF** = 100

Projection for konec > Max = 50

Example



- positioning the decimal point does not have effect on display projection
- after confirmation of the value the decimal point automatically moves to max. number of decimal places



FD_r

Setting projection of decimal point

- positioning of decimal point in measuring mode on the display is set here

- **DEF** = 00.0

Projection of decimal point on the display > XXX.x Example

000

◀

000

▶

000

* following item of the menu depends on instrument equipment

30

Calibration of the beginning and the end of range of linear potentiometer is on page 31





ARR Setting display projection for maximum value of input signal

- positioning the decimal point does not have effect on display projection
- after confirmation of the value the decimal point automatically moves to max. number of decimal places
- range of the setting is ± 1999
- **DEF** = 100

Projection for 105 Ohm > Max = 350 Example

+ 100.0	+ 100.0	+ 10.0	+ 10.0	+ 10.0	+ 10.0
+ 10.0	+ 10.0	+ 1.0	+ 1.0	+ 1.0	+ 1.0
+ 0.35.0	+ 0.35.0	+ 0.35.0	+ 0.35.0	FO_r	



FO_r Setting projection of decimal point


- positioning of decimal point in measuring mode on the display is set here
- **DEF** = 00.0

Projection of decimal point on the display > XXX.x Example

000	00.0	00.0	FO_r	
-----	------	------	------	--

* following item of the menu depends on instrument equipment

OM 351RTD


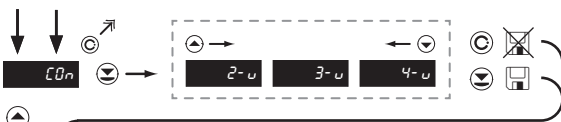
**CO n** Selecting the type of sensor connection

- in 2- or 3- wire connection it is necessary to link the unconnected inputs (see Chapter Connection)
- **DEF** = 4-w

Menu	Connection
2-w	2-wire
3-w	3-wire
4-w	4-wire

Type of connection - 3-wire > CO n = 3-w

Example

**FD r** Setting projection of decimal point

- positioning of decimal point in measuring mode on the display is set here

- 000. > measuring range -50°...400°C
- 00.0 > measuring range -50,0°...199,9°C
- **DEF** = 00.0

Projection of decimal point on the display > XXX.x

Example



* following item of the menu depends on instrument equipment

RTD RTD RTD RTD RTD RTD RTD RTD RTD RTD RTD RTD RTD RTD RTD

OM 351T/C



00d Selection of type of thermocouple

- setting the input range depends on ordered measuring range

- DEF = B
- DEF = S
- DEF = K

Menu	Type „A“	Type „B“	Type „C“
B	B		
R		R	
S		S	
T		T	
E			E
J			J
K			K
N			N

Type of thermocouple "K" Example

ε J T 0.1



C0n Setting the method of evaluation of the cold junction

- DEF = In. 1

Menu	Reference thermocouple	Description
In. 1	No	measurement of cold junction on instrument brackets
In. 2	Yes	measurement of cold junction on instrument brackets with anti-series connection of reference thermocouple
E. 1	No	the whole measuring system is working under the same and constant temperature
E. 2	Yes	upon the use of compensation box

Method and process of setting and using cold junctions is on page 50

Measurement of cold junction on instrument brackets > C0n = In. 1 Example

In. 1 E.E.d



t.C.J. Setting the temperature of the cold junction - **DEF** = 60

- range of the setting is 0°...60°C

Temperature of the cold junction > t.C.J. = 25 Example

000	001	002	003	004	005
006	006	005	025	025	025
025	noU	* following item of the menu depends on instrument equipment			

30

! For thermocouple type "B" the items CO and t.C.J. are not accessible

T/C T/C T/C T/C T/C T/C T/C T/C T/C T/C



L 1 Setting the boundary for limit 1

- range of the setting is ± 1999
- presetting "Hysteresis"=0 "Delay"=0

- contingent change of hysteresis or offset of the switch-on may be performed in the PROFi menu

- **DEF** = 25

Nastavení limity 1 > L1 = 30

Example



L 2 Setting the boundary for limit 2

- range of the setting is ± 1999
- presetting "Hysteresis"=0 "Delay"=0

- contingent change of hysteresis or delay of the switch-on may be performed in the PROFi menu

- **DEF** = 75

Nastavení limity 2 > L2 = 230

Example



Items for "Limits" and "Analog output" are accessible only if the instrument contains them.

TYPE Setting the type of analog output - DEF = E 4

Menu	Range	Description
i20	0...20 mA	
E 4	4...20 mA	with indication of error statement (<3,6 mA)
i 4	4...20 mA	
i 5	0...5 mA	
U 2	0...2 V	
U 5	0...5 V	
U 10	0...10 V	

Type of analog output - 0...10 V > Type = U 10 Example

R.Lo Assigning the displayed value to the end of the analog output range - DEF = 0; 40 (RTD, T/C)

- range of the setting is ± 1999

Display projection for the beginning of AO range > A.Lo = 0 Example

R.Hi Assigning the displayed value to the end of the analog output range - DEF = 100; 199.9 (RTD, T/C)

- range of the setting is ± 1999

Display projection for the end of AO range > A.Hi = 120 Example



MENU Setting the menu type LIGHT/PROFI

LIG > LIGHT menu, a simple menu, which contains only items necessary for instrument setting
> linear structure of the menu

PRO > PROFIL menu, a complete menu for entire instrument setting
> tree structure of the menu

- **DEF** = LIG

Menu LIGHT > MENU = LIG

Example

LIG



rES Restoration of the instrument manufacture setting

- in case of incorrect setting or calibration it

is possible to return to manufacture setting. Prior execution of the changes you will be asked to confirm your selection (YES)
- reading the manufacture calibration and original setting of items in the menu

Obnova výrobního nastavení > rES


Example

rES

* following item depends on the instrument type, for OM 351DU > "CLo"

OM 351AC		32
OM 351DC		32
OM 351PM		32
OM 351DU		31
OM 351OHM		32
OM 351RTD		32
OM 351T/C		32

OM 351DU

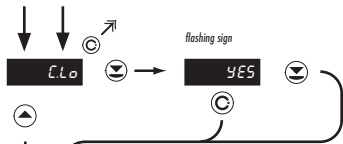


C.Lo Input range calibration - potentiometer slider is in its initial position Only for type OM 351DU

- prior confirmation of the flashing sign "Yes" the potentiometer slider has to be in given position of rest

Calibration of the beginning of the range > C.Lo Example

YES

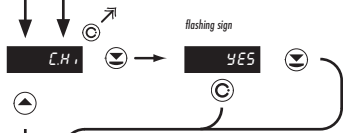


C.Hi Input range calibration - potentiometer slider is in its initial position Only for type OM 351DU

- prior confirmation of the flashing sign "Yes" the potentiometer slider has to be in given position of rest

Calibration of the end of the range > C.Hi Example

YES

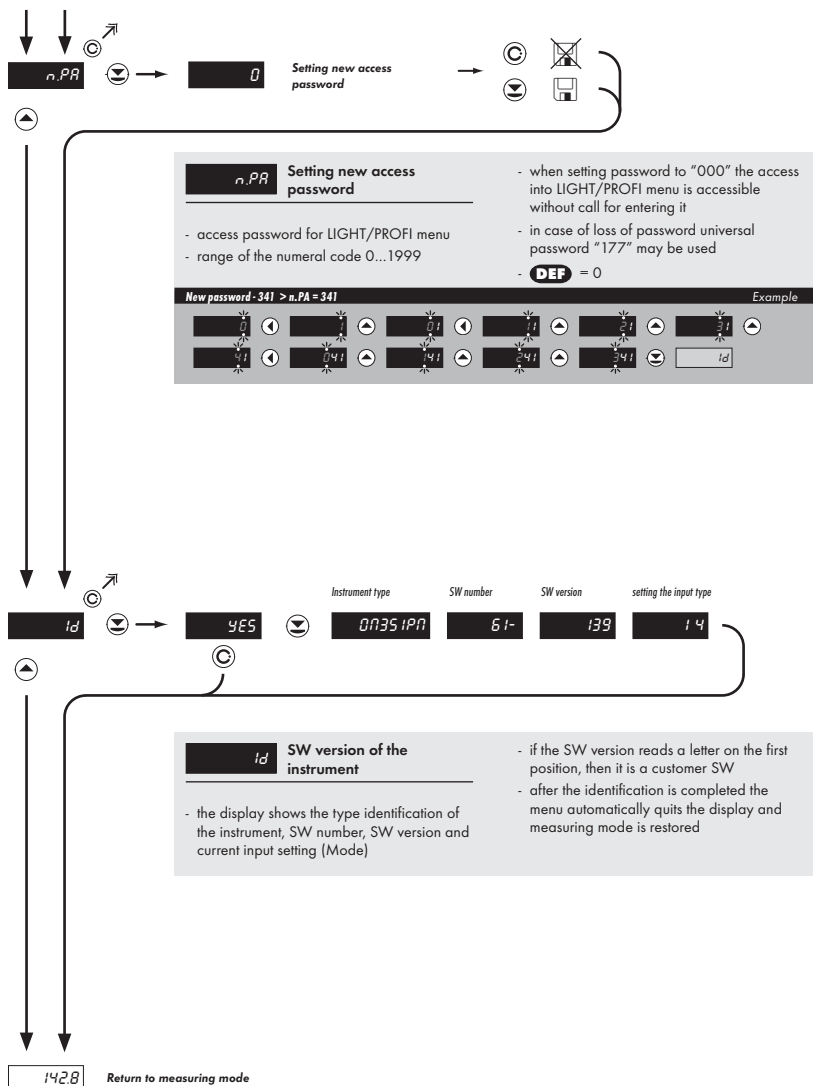

PROFI

Kompletni programovací menu

- contains complete instrument menu and is protected by an optional numeral code
- designed for expert users
- preset from manufacture is **LIGHT** menu


SETTING
PROFI


profi

- For expert users
- Complete instrument menu
- Access is password protected
- Possibility to arrange items of the „User“ menu
- Tree menu structure

SWITCHING OVER TO "PROFI" MENU


- Ⓞ + ▼
 - temporary switch-over to **PROFI** menu, which is suitable to edit a few items
 - after quitting **PROFI** menu the instrument automatically switches to **LIGHT** menu
 - access is password protected
- Ⓞ + ☺
 - access into **LIGHT** menu and transition to item „MnU“ with subsequent selection of „PRO“ and confirmation
 - after re-accessing the menu the **PROFI** type is active
 - access is password protected

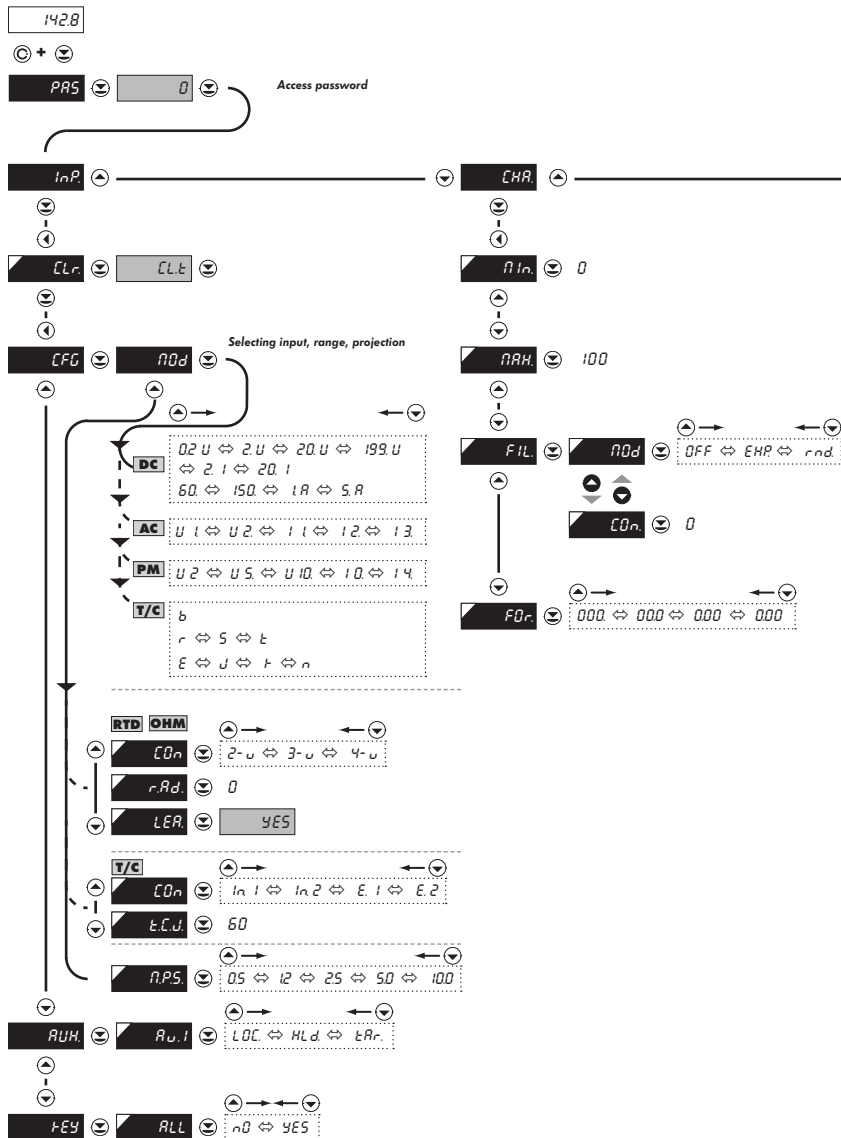

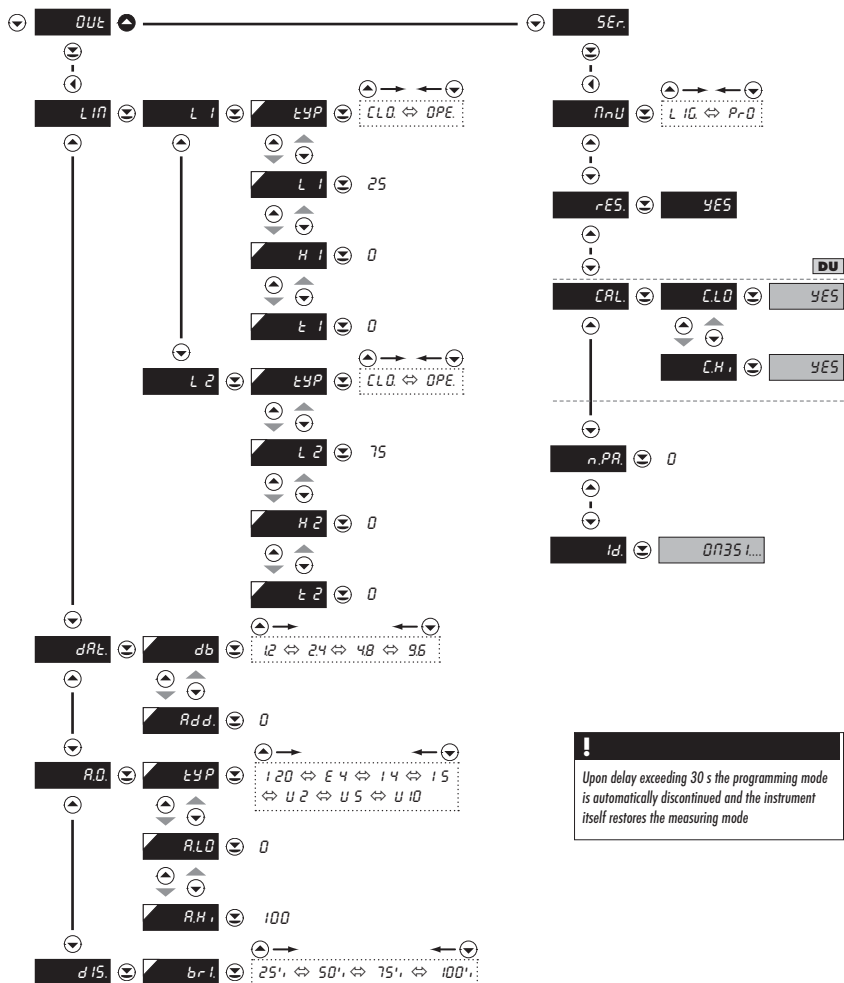

!
 Upon delay exceeding 30 s the programming mode is automatically discontinued and the instrument itself restores the measuring mode



6.1 SETTING "PROFI" - INPUT



The basic instrument parameters are set in this menu

- CLR** Tare resetting
- CFG** Selecting the measuring range and rate
- AUM** Setting the external input function
- FEY** Setting the ENTER key function

6.1.1 TARE RESETTING



6.1.2a SELECTING THE INSTRUMENT MEASURING RANGE

Navigation icons: ↑, ←, →, ↓, and a menu icon.

inP	CL. t.	nOd	DC - 1	0.2 U	DC - 2	60
CHR.	CFG	n.P.S.		2. U		150
OUT.	AUX.	DEF		20. U	DEF	1. A
SEr.	KEY			199. U		5. A
				2. I		
				20. I		
			T/C		AC	
			b		U 1	DEF
			r		U 2	
		DEF	S		1. I	
			t		1. 2	
			ε		1. 3	
			J			
		DEF	F		PM	
			n		U 2	
					U 5	
					U 10	
					1. 0	
					1. 4	DEF

nOd Selecting the instrument measuring range

- setting the input range depends on ordered measuring range

Menu	Range „S“	Range „U“
U 1.	0...10 V	0...250 V
U 2.	0...120 V	0...450 V

Menu	Range „K“	Range „P“
I 1.	0...60 mV	0...1 A
I 2.	0...150 mV	0...2,5 A
I 3.	0...300 mV	0...5 A

Menu	Range „A“	Range „B“
0.2U	±0,2 V	
2.U	±2 V	
20.U	±20 V	
199.U	±199 V	
2. i	±2 mA	
20. i	±20 mA	
60.		±60 mV
150.		±150 mV
1. A		±1 A
5. A		±5 A

Menu	Range
U 2.	0...2 V
U 5.	0...5 V
U 10.	0...10 V
I 0.	0...20 mA
I 4.	4...20 mA

Menu	Type „A“	Type „B“	Type „C“
B	B		
R		R	
S		S	
T		T	
E			E
J			J
K			K
N			N

6.1.2b SETTING THE SENSOR CONNECTION

RTD OHM


CO_n Selecting the sensor connection

- in 2- or 3- wire connection it is necessary to link the unconnected inputs (see Chapter Connection)


 2-wire connection

 3-wire connection

 4-wire connection

6.1.2c OFFSET OF THE BEGINNING OF THE RANGE


RTD OHM


r.Ad Offset of the beginning of the measuring range

- in cases when it is necessary to shift the beginning of the range by certain value, e.g. when sensor is used in a measuring head
- entered directly in Ohm (0...19,99)
- **DEF** = 0


6.1.2d COMPENSATION OF 2-WIRE CONDUCT

RTD OHM

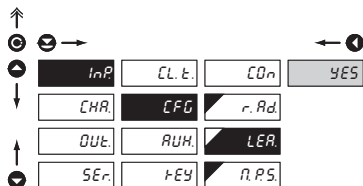
LER Compensation of 2-wire conduct

- for measurement accuracy it is necessary to perform compensation of the conduct always in case of 2-wire connection
- prior to confirmation of the displayed challenge „YES“ it is necessary to substitute the sensor at the end of the conduct by a short circuit
- **DEF** = 0

6.1.2e SETTING THE METHOD OF EVALUATION OF THE COLD JUNCTION

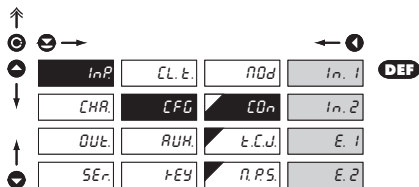T/G


CO_n Method of evaluation of the cold junction

In.1 Measurement without reference thermocouple

- cold junction measurement on the instrument brackets

In.2 Measurement with reference thermocouple

- cold junction measurement on the instrument brackets with anti-series connection of ref. thermocouple

E.1 Measurement without reference thermocouple

- the whole measuring system is working under the same and constant temperature


E.2 Measurement with reference thermocouple

- upon the use of compensation box



Description of the method of evaluation of the cold junction is in chapter 8, page 56


6.1.2f TEMPERATURE OF THE COLD JUNCTION

T/G


t.C.J. Setting the temperature of the cold junction


- range 0...60°C with compensation box
- **DEF** = 60°C

6.1.2g MEASURING RATE

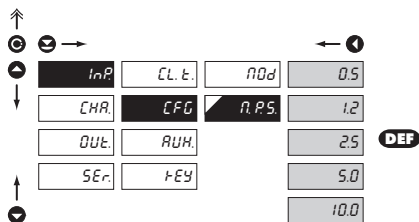
n.P.S. Setting the measuring rate

0.5	Rate - 0,5 meas./s
1.2	Rate - 1,2 meas./s
2.5	Rate - 2,5 meas./s
5.0	Rate - 5 meas./s
10.0	Rate - 10 meas./s

6.1.3 EXTERNAL INPUT FUNCTION SELECTION

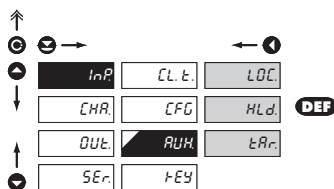

AUH. External input function selection

LDC.	LOCK, locking the control keys on the instrument
HLd.	HOLD, stop measuring of the entire instrument
tAR.	TARA - Tare activation*

*

Only for type DC, PM

6.1.4 OPTIONAL ACCESSORY FUNCTIONS OF THE KEYS

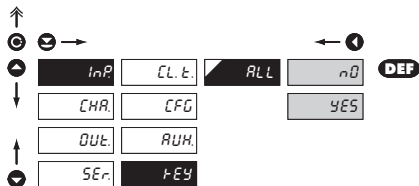

FEY Setting other functions of the control-keys

ALL Setting all keys

- owing to limited space in the instrument's memory it is not feasible to set the keys' functions one by one

n0 Accessory functions are off

YES Accessory functions are on


! Tare value displayed

☺ Display taring



Only for type DC, PM

6.2 SETTING "PROFI" - CHANNELS



In this menu the instrument input parameters are set

nIn Setting display projection for minimum value of input signal ①

nRH Setting display projection for maximum value of input signal ②


FIL. Setting the digital filters ③

FDr. Setting the decimal point ④

Input type	Setting options
DC	① ② ③ ④
AC	① ② ③ ④
PM	① ② ③ ④
DU	① ② ③ ④
OHM	① ② ③ ④
RTD	③ ④
T/C	③

6.2.1 PROJECTION ON THE DISPLAY

DC AC PM DU OHM




nIn Setting display projection for minimum value of input signal

- range of the setting is ± 1999
- **DEF** = 0

nRH Setting display projection for maximum value of input signal

- range of the setting is ± 1999
- **DEF** = 100

6.2.3 DIGITAL FILTERS

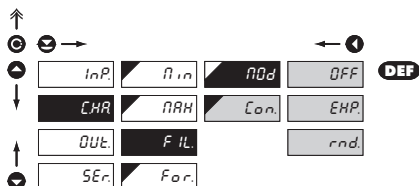

FIL. Setting the digital filters

- the instrument allows for classic projection of a number with decimal point as well as with floating DP, allowing for projection of a number in its most precise form "FLP."

Con. Setting the constant

- this menu item is always displayed after selection of a particular type of filter

EHP. Selection of exponential filter


- the value is calculated from a number of measurements selected in „CON“
- range 2...100

nod. Selection of value round-up

- it is set by ...arbitrary number, which determines the projection step (e.g.: "Con"=2,5 > display 0, 2.5, 5,...)

6.2.4 DECIMAL POINT

DC AC PM DU OHM RTD

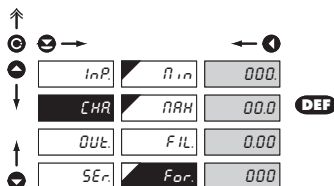

For. Setting the decimal point

- the instrument allows for classic projection of a number with placement of the decimal point


000. Setting the DP - XXXX.

000. Setting the DP - XXX.x

0.00 Setting the DP - XX.xx

000 Setting the DP - X.xxx

6.3 SETTING „PROFI“ - OUTPUTS



It is possible to set the parameters of the instrument output signals in this menu

L IN Setting the type and the switching of limits

dARt Setting the type and the parameters of data output


R. D. Setting the type and parameters of analog output

d IS. Setting the display brightness



Analog and data outputs may not be fitted simultaneously

6.3.1α LIMITS - RELAY FUNCTIONS

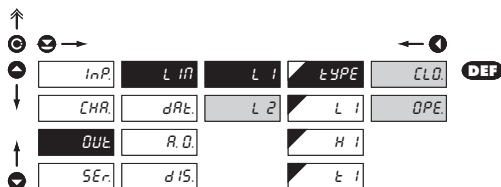


TYPE Setting the type of relay function

CLD. Relay switches on when the condition is met

OPE. Relay switches off when the condition is met

6.3.1b LIMITS - BOUNDARIES

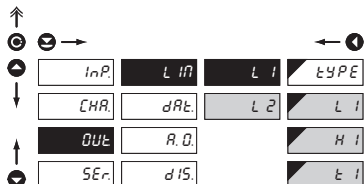

L 1 Setting the boundaries

L 1 Setting the boundary for relay switch-on

- within the full display range (± 1999)
- **DEF** = 25 (L 1), 75 (L 2)

H 1 Setting hysteresis

- within the full display range (± 1999)
- **DEF** = 0


t 1 Setting the offset of the relay switch-on

- within the range 0...99,9 s
- **DEF** = 0

?

The process of setting the Limit 2 is identical with the setting for Limit 1


6.3.2a DATA OUTPUT - RATE

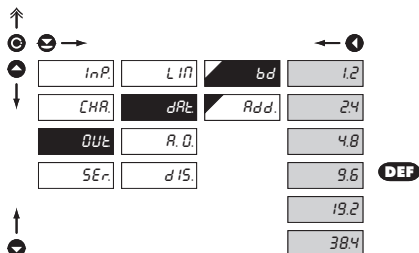

bd Setting the data output rate


- 1.2** Rate - 1 200 Baud
- 2.4** Rate - 2 400 Baud
- 4.8** Rate - 4 800 Baud
- 9.6** Rate - 9 600 Baud
- 19.2** Rate - 19 200 Baud
- 38.4** Rate - 38 400 Baud

6.3.2b DATA OUTPUT - ADDRESS


Rdd. Setting the instrument address


- setting within the range 0...31
- **DEF** = 00

6.3.3a ANALOG OUTPUT - TYPE

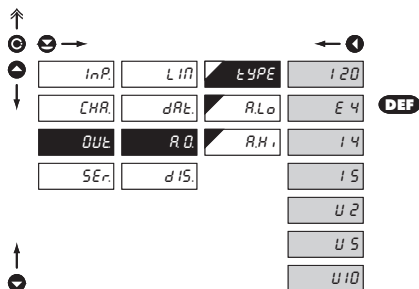
tYPE Setting the type of analog output

- | | |
|--|------------------|
| 120 | Type - 0...20 mA |
| ε 4 | Type - 4...20 mA |
| - with indication of error statement (<3,6 mA) | |
| 14 | Type - 4...20 mA |
| 15 | Type - 0...5 mA |
| U 2 | Type - 0...2 V |
| U 5 | Type - 0...5 V |
| U 10 | Type - 0...10 V |

6.3.3b ANALOG OUTPUT - RANGE



R.O. Setting the analog output range

- analog output is isolated and its value corresponds with the displayed data. It is fully programmable, i.e. it allows to assign the AO limit points to any two arbitrary points of the entire measuring range


R.Lo Assigning the displayed value to the beginning of the analog output range

- range of the setting is ± 1999
- **DEF** = 0, -40 (RTD, T/C)

R.Hi Assigning the displayed value to the end of the analog output range

- range of the setting is ± 1999
- **DEF** = 100, 199,9 (RTD, T/C)

6.3.4 DISPLAY BRIGHTNESS

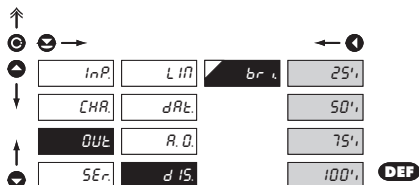

br. Setting the display brightness

- by selecting the display brightness we may react properly to light conditions in place of location of the instrument
- brightness in the programming menu is always 100 %


25% Display brightness - 25 %

50% Display brightness - 50 %

75% Display brightness - 75 %

100% Display brightness - 100 %


6.4 SETTING "PROFI" - SERVICE



The instrument's service functions are set in this menu

- n.n.U.** Selection of menu type LIGHT/PROFI
- r.ES.** Restoration of the manufacture setting and instrument calibration
- CAL.** Calibration of input range for verion „DU“
- n.PR.** Setting new access password
- .d.** Instrument identification

6.4.1 SELECTION OF THE TYPE OF PROGRAMMING MENU

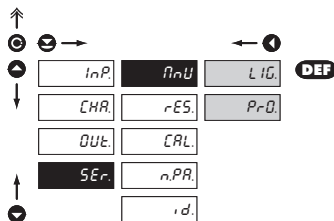

n.n.U. Selection of menu type LIGHT/PROFI

- allows to set the menu complexity as per user needs and abilities


L.L.G. Active LIGHT menu

- simple programming menu, contains only items necessary for instrument configuration and setting
- linear menu structure > items in succession

PR.D. Active PROFI menu

- complete programming menu for expert users
- tree menu

6.4.2 RESTORATION OF THE MANUFACTURE SETTING




rES. Restoration of the instrument manufacture setting

- in case of incorrect setting or calibration it is possible to return to manufacture setting. Prior execution of the changes you will be asked to confirm your selection „YES“
- reading the manufacture calibration and original setting of items in the menu (DEF)

6.4.3 CALIBRATION OF THE INPUT RANGE


DU

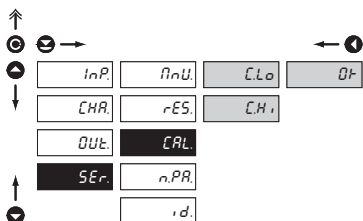

CARL. Calibration of the input range

- when MIN is displayed move the potentiometer slider into required minimum position and confirm by „Enter“, calibration is confirmed by showing sign „OK“
- when MAX is displayed move the potentiometer slider into required maximum position and confirm by „Enter“, calibration is confirmed by showing sign „OK“


6.4.4 SETTING NEW ACCESS PASSWORD



n.PR. Setting new password for access into the LIGHT and PROFi menu


- this option allows to change the numeral code, which protects the access into the LIGHT and PROFi Menu.
- numeral code range is 0...1999
- universal password in case of loss „177“

6.4.5 INSTRUMENT IDENTIFICATION


id. Projection of instrument SW version

- the display shows the type identification of the instrument, SW number, SW version and current input setting (Mode)
- if the SW version reads a letter on the first position, then it is a customer SW
- after the identification is completed the menu automatically quits the display and measuring mode is restored

7.0 "USER" MENU CONFIGURATION

- **USER** menu is designed for users who need to change only several items of the setting without the option to change the basic instrument setting (e.g. repeated change of limit setting)
- there are no default items from manufacture in **USER** menu
- menu configuration possible on items indicated by inverse triangle  L I
- setting may be performed in **LIGHT** or **PROFI** menu, with the **USER** menu then overtaking the given menu structure



- For user operation
- Menu items are set by the user (Profi/Light) as per request
- Access is not password protected

SETTING

flashing sign - current setting is displayed



n0

item will not be displayed in USER menu


YES

item will be displayed in USER menu with the chance of editing

SHD

item will be solely displayed in USER menu

An instrument with input for temperature measurement with thermocouple allows for setting of two types of measurement of the cold junction.

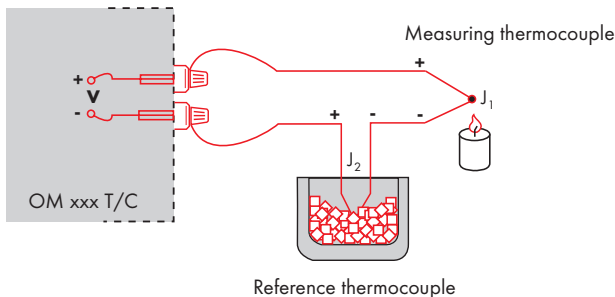

WITH REFERENCE THERMOCOUPLE

- a reference thermocouple may be located in the same place as the measuring instrument or in place with stable temperature/compensation box
- when measuring with reference thermocouple set $\mathcal{L}\mathcal{J}\mathcal{L}$ in the instrument menu to $i_{r,2}$ or $\mathcal{E},2$
- when using a thermostat (a compensation box or environment with constant temperature) set in the instrument menu $\mathcal{L}\mathcal{J}\mathcal{L}$ its temperature (applies for setting $\mathcal{L}\mathcal{J}\mathcal{L}$ to $\mathcal{E},2$)
- if the reference thermocouple is located in the same environment as the measuring instrument then set in the instrument menu $\mathcal{L}\mathcal{J}\mathcal{L}$ to $i_{r,2}$. Based on this selection the measurement of the surrounding temperature is performed by a sensor located in the instrument terminal board.

WITHOUT REFERENCE THERMOCOUPLE

- inaccuracy originating from the creation of dissimilar thermocouples on the transition point terminal-conductor of the thermocouple is not compensated for in the instrument
- when measuring without reference thermocouple set $\mathcal{L}\mathcal{J}\mathcal{L}$ in the instrument menu to $i_{r,1}$ or $\mathcal{E},1$
- when measuring temperature without reference thermocouple the error in the measured data may be even 10°C (applies for setting $\mathcal{L}\mathcal{J}\mathcal{L}$ to $\mathcal{E},1$)

The instruments communicate via serial line RS232 or RS485. For communication they use the ASCII protocol. Communication runs in the following format:

ASCII: 8 bit, no parity, one stop bit

The transfer rate is adjustable in the instrument menu and depends on the control processor used. The instrument address is set in the instrument menu in the range of 0 + 31. The manufacture setting always presets the ASCII protocol, rate of 9600 Baud, address 00. The type of line used - RS232 / RS485 - is determined by an exchangeable card automatically identified by the instrument.

COMMANDS FOR INSTRUMENT OPERATION

The commands are described in specification you can find at www.orbit.merret.cz/rs. A command consists of a number and a letter. The size of the letters have a significance.

DETAILED DESCRIPTION OF COMMUNICATION VIA SERIAL LINE

Activity	Type	Protocol	Data transferred														
Data solicitation (PC)	232	ASCII	#	A	A	<CR>											
	485	ASCII	#	A	A	<CR>											
Data transfer (Instrument)	232	ASCII	>	R	SP	D	D	D	D	D	(D)	(D)	<CR>				
	485	ASCII	>	R	SP	D	D	D	D	D	(D)	(D)	<CR>				
Command transfer (Instr.) - identification	232	ASCII	#	A	A	1	Y	<CR>									
	485	ASCII	#	A	A	1	Y	<CR>									
Command confirmation (Instrument)	232	ASCII	ok	!	A	A	<CR>										
			bad	?	A	A	<CR>										
	485	ASCII	ok	!	A	A	<CR>										
			bad	?	A	A	<CR>										

Legend			
#	35	23 _H	Beginning of the command
A	A	0...31	Two signs of the inst. address (sent in ASCII - decades and units, ex."01")
<CR>	13	0D _H	Carriage return
<SP>	32	20 _H	Space
N	P		Number and command - command code
D			Data - usually signs "0"..."9",",","."; (D) - dp. and (-) may prolong data
R		30 _H ...3F _H	Relay status; zero bit corresponds with 1st relay, 1st bit with 2nd relay, etc.
!	33	21 _H	Positive command confirmation (ok)
?	63	3F _H	Negative command confirmation (bad)
>	62	3E _H	Beginning of the transmitted data

ERROR	CAUSE	ELIMINATION
<i>E. d.U</i>	Number is too small (large negative) to be displayed	change DP setting, channel constant
<i>E. d.O.</i>	Number is too large to be displayed	change DP setting, channel constant
<i>E. t.U</i>	Number is outside the table range	increase the table values, change input setting (channel constant)
<i>E. t.O.</i>	Number is outside the table range	increase the table values, change input setting (channel constant)
<i>E. i.U</i>	Input quantity is smaller than permitted input quantity range	change input signal value or input (range) setting
<i>E. i.O.</i>	Input quantity is larger than permitted input quantity range	change input signal value or input (range) setting
<i>E. H_U</i>	A part of the instrument does not work properly	send the instrument for repair
<i>E. EE</i>	Data in EEPROM corrupted	perform restoration of manufacture setting, upon repeated error statement send instrument for repair
<i>E. dt</i>	Data in EEPROM outside the range	perform restoration of manufacture setting, upon repeated error statement send instrument for repair
<i>E. CL.</i>	Memory was empty (presetting carried out)	upon repeated error statement send instrument for repair, possible failure in calibration

INPUT

selectable in configuration menu

			DC
DC 1	±2 mA	< 200 mV	Input 1
	±20 mA	< 200 mV	Input 1
	±200 mV	100 kOhm	Input 2
	±2 V	100 kOhm	Input 2
	±20 V	10 MOhm	Input 3
DC 2	±1 A	< 150 mV	Input 1
	±5 A	< 150 mV	Input 1
	±60 mV	100 kOhm	Input 2
	±150 mV	100 kOhm	Input 2

range is fixed, as per order

			AC
Range U:	0...10 V	100 kOhm	Input 2
	0...120 V	10 MOhm	Input 3
	0...250 V	10 MOhm	Input 2
	0...450 V	10 MOhm	Input 3
Range I:	0...60 mV	100 kOhm	Input 1
	0...150 mV	100 kOhm	Input 1
	0...300 mV	100 kOhm	Input 1
	0...1 A	< 150 mV	Input 1
	0...5 A	< 150 mV	Input 1

selectable in configuration menu

			PM
DC 1	0/4...20 mA	< 400 mV	Input 1
	0...2 V	1 MOhm	Input 2
	0...5 V	1 MOhm	Input 3
	0...10 V	1 MOhm	Input 3

range is fixed, as per order

			OHM
DC 1	0...200 Ohm		
	0...2 kOhm		
	0...20 kOhm		
	0...100 kOhm		
	5...105 Ohm		
Connection:	2, 3 or 4-wire		

Pt xxxx	-50,0°...199,9°C/-50,0°...400°C
Ni xxxx	-30,0°...199,9°C
Type Pt:	100/500/1 000 Ohm, platinum couple s $\alpha = 0,003850 \text{ Ohm}/\text{Ohm}/\text{°C}$
Type Ni:	Ni 1 000, 5000 ppm/6180 ppm
Connection:	2, 3 or 4-wire

selectable in configuration menu

Type:			T/C
J (Fe-CuNi)	-200°...900°C		
K (NiCr-Ni)	-200°...1 300°C		
T (Cu-CuNi)	-200°...400°C		
E (NiCr-CuNi)	-200°...690°C		
B (PtRh30-PtRh6)	300°...1 820°C		
S (PtRh10-Pt)	-50°...1 760°C		
R (Pt13Rh-Pt)	-50°...1 740°C		
N (Omegaalloy)	-200°...1 300°C		

Lin. pot.supply 2,5 VDC/6 mA
min. potentiometer resistance is 500 Ohm

PROJECTION

Display:	1999, intensive red or green 7-segment LED, digit height 14 mm
Projection:	±1999
Decimal point:	adjustable - in programming mode
Brightness:	adjustable - in programming mode

INSTRUMENT ACCURACY

Temperature coef.:	100 ppm/°C	
Accuracy:	±0,2% of the range + 1 digit ±0,3 % of the range + 1 digit	T/C, AC
Resolution:	0,1° 1°C	RTD T/C
Rate:	0,5 - 1,2 - 2,5 - 5 - 10 measurements/s	
Overload capacity:	10x (t < 100 ms), 2x (long-term)	
Digital filter	adjustable in configuration menu	
Comp.of conduct:	max. 40 Ohm	RTD
Comp.of cold junct.:	adjustable 0°...98°C or automatic (99)	T/C
Functions:	Tare - display resetting Hold - stop measuring (upon contact) Lock - control keys locking	
OM Link:	Company communication interface for instrument operation, setting and update	
Watch-dog:	reset after 25 ms	
Calibration:	at 25°C and 40 % r.h.	

COMPARATOR

Type:	digital, adjustable in the menu
Limits:	±1999
Hysteresis:	0...999
Delay:	0...99,9 s
Outputs:	2x relays with switch-on contact (230 VAC/30 VDC, 3 A)*
Relay:	1/8 HP 277 VAC, 1/10 HP 125 V, Pilot Duty D300

* values apply for resistance load

DATA OUTPUTS

Protocols:	ASCII
Data format:	8 bit + no parity + 1 stop bit (ASCII)
Rate:	1 200...38 400 Baud
RS 232:	isolated, two-way communication
RS 485:	isolated, two-way communication, addressing (max. 31 instruments)

- cannot be combined with analog output

ANALOG OUTPUTS

Type:	isolated, programmable with resolution of max. 4 000 points, analog output corresponds with the displayed data, type and range are adjustable
Non-linearity:	0,2 % of the range
TC:	100 ppm/°C
Rate:	response to change of value < 250 ms
Voltage:	0...2 V/5 V/10 V
Current:	0...5/20 mA/4...20 mA - compensation of conduct up to 500 Ohm

- cannot be combined with data output

EXCITATION

Adjustable:	10...15 VDC/40 mA, isolated
-------------	-----------------------------

- cannot be combined with data/analog output

POWER SUPPLY

Options:	24/110/230 VAC, 50/60 Hz, ±10 %, 3 VA 12...24 VDC/max. 150 mA, nonisolated - only in basic version (without AO, PN and RS xxx) and upon request 10...30 VDC/max. 250 mA, isolated
Protection:	by a fuse inside the instrument VAC (T 80 mA), VDC (T 630 mA)

MECHANIC PROPERTIES

Material:	Noryl GFN2 SE1, incombustible UL 94 V-I
Dimensions:	96 x 48 x 120 mm
Panel cut-out:	90,5 x 45 mm

OPERATING CONDITIONS

Connection:	connector terminal board, conductor section up to 2,5 mm ²
Stabilisation period:	within 15 minutes after switch-on
Working temp.:	0°...60°C
Storage temp.:	-10°...85°C
Cover:	IP65 (front panel only)
Construction:	safety class I
El. safety:	EN 61010-1, A2
Insul. resistance:	for pollution degree II, measuring cat. III. AC power supply > 600 V (ZI), 300 V (DI) DC power supply, input, output, exc. > 300 V (ZI), 250 V (DI)


EMC:	EN 61000-3-2+A12; EN 61000-4-2, 3, 4, 5, 8, 11; EN 550222, A1, A2
------	--

ZI - Primary insulation, DI - Double insulation


Front view



Panel cut





Side view



Panel thickness: 0,5...20 mm

Instrument installation

1. insert the instrument into the panel cut-out
2. fit both travellers on the box
3. press the travellers close to the panel

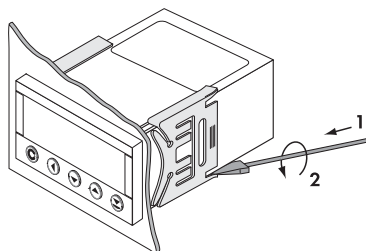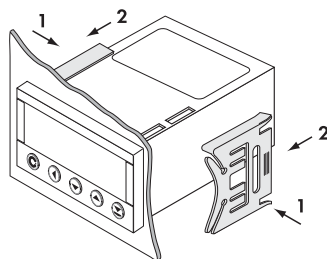

Instrument disassembly

1. slide a screw driver under the traveller wing
2. turn the screw driver and remove the traveller
3. take the instrument out of the panel

Product **OM 351 DC AC PM DU RTD T/C OHM**
 Type
 Manufacturing No.
 Date of sale

A guarantee period of 24 months from the date of sale to the user applies to this instrument.


Defects occurring during this period due to manufacture error or due to material faults shall be eliminated free of charge.

For quality, function and construction of the instrument the guarantee shall apply provided that the instrument was connected and used in compliance with the instructions for use.

The guarantee shall not apply to defects caused by:

- mechanic damage
- transportation
- intervention of unqualified person incl. the user
- unavoidable event
- other unprofessional interventions

The manufacturer performs guarantee and post.guarantee repairs unless provided for otherwise.

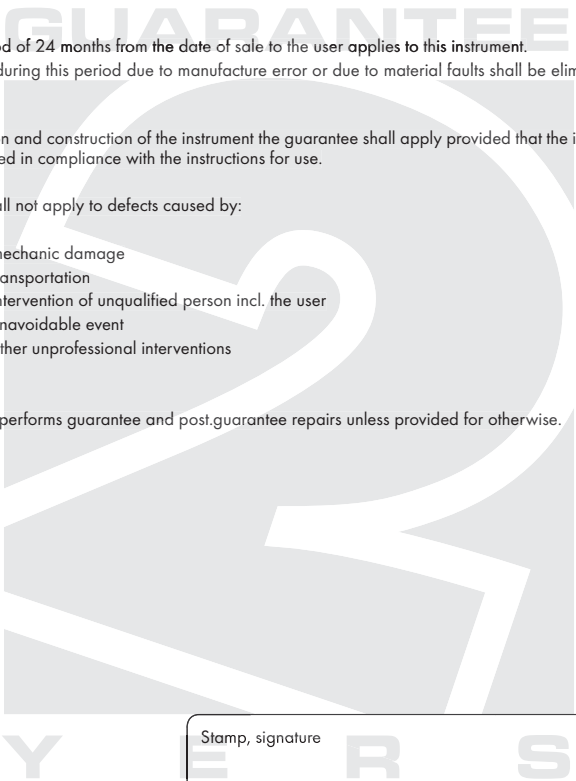

Stamp, signature

DECLARATION OF CONFORMITY

Company: **ORBIT MERRET, spol. s r.o.**
Klánská 81/141, 142 00 Prague 4, Czech Republic, IDNo: 00551309

Manufactured: **ORBIT MERRET, spol. s r.o.**
Vodňanská 675/30, 198 00 Prague 9, Czech Republic

declares at its full responsibility that the product presented hereunder meets all technical requirements, is safe for use when utilised under the terms and conditions determined by ORBIT MERRET, spol.s r.o. and that our company has taken all measures to ensure conformity of all products of the type listed hereunder, which are being brought out to the market, with technical documentation and requirements of the appurtenant statutory orders.

Product: 3 ½ -digit programmable panel instrument

Type: **OM 351**

Version: DC, PM, AC, RTD, T/C, DU, OHM, UC

Conformity is assessed pursuant to the following standards:

Electrical safety:	EN 61010-1	
EMC:	EN 50131-1, chapter 14 and chapter 15	
	EN 50130-4, chapter 7	EN 61000-4-11
	EN 50130-4, chapter 8	EN 61000-4-11
	EN 50130-4, chapter 9	EN 61000-4-2
	EN 50130-4, chapter 10	EN 61000-4-3
	EN 50130-4, chapter 11	EN 61000-4-6
	EN 50130-4, chapter 12	EN 61000-4-4
	EN 50130-4, chapter 13	EN 61000-4-5
	EN 50130-5, chapter 20	
	prEN 50131-2-1, par. 9.3.1	
	EN 61000-4-8	
	EN 61000-4-9	
	EN 61000-3-2 ed. 2:2001	
	EN 61000-3-3: 1997, Cor. 1:1998, Z1:2002	
	EN 55022, chapter 5 and chapter 6	

and government ordinance:

Electrical safety: No. 168/1997 Sb.

EMC: No. 169/1997 Sb.

The evidence are the protocols of authorized and accredited organization:

VTÚE Praha, experimental laboratory No. 1158, accredited by ČIA
VTÚPV Vyškov, experimental laboratory No. 1103, accredited by ČIA

Place and date of issue: Prague, 18. December 2003

Miroslav Hackl
Company representative

Mode of asses. of conformity: §12, par. 4 b, d of Act No. 22/1997 Sb.